

## BEIGE A1

TOP DYEING - 2%



SPLIT - 3%



PENETRATION




60° Solubility	Penetration	Light	F A S T N E S S					
			PERSPIRATION			WASHING		
			CS	SC	SW	CS	SC	SW
50	4	4	2	2	3	4	3	3

SCALE - 1 TO 5  
 CS - COTTON + SILK  
 SC - SPUN DIACETATE  
 SW - SPUN WOOL

# Spectrum Peak Pick Report

02-04-2019 03:30:56 PM

Data Set: BEIGE A1 B-2018-182 10PPM - RawData

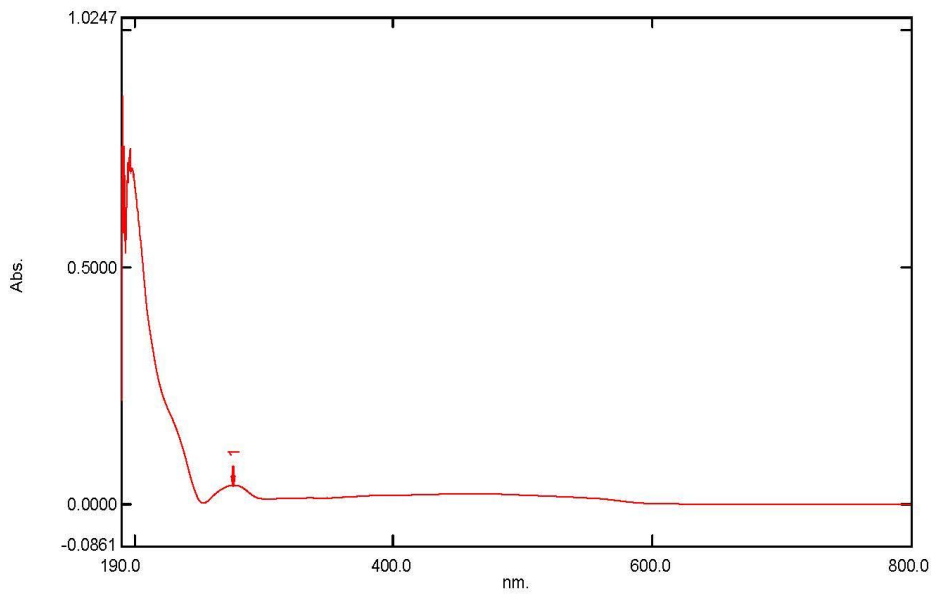

[Measurement Properties]  
Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1		276.0	0.0395	

[Instrument Properties]  
Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

[Attachment Properties]  
Attachment: None


[Operation]  
Threshold: 0.0010000  
Points: 4  
InterPlate: Disabled  
Average: Disabled

[Sample Preparation Properties]  
Weight: 0.1  
Volume: 100  
Dilution: 10 ppm  
Path Length:  
Additional Information:

# Spectrum Peak Pick Report

02-04-2019 03:33:25 PM

Data Set: BEIGE A1 B-2018-182 20PPM - RawData

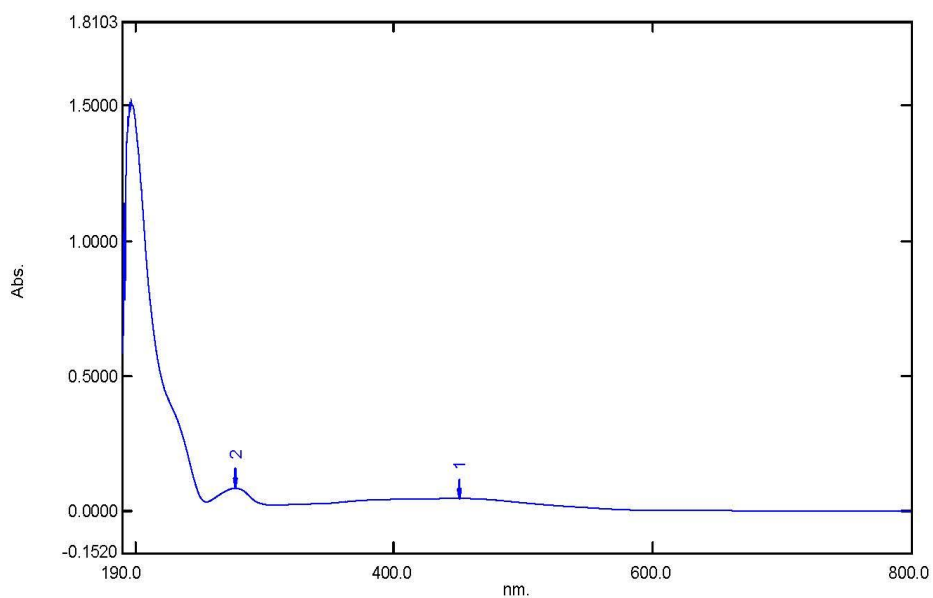

#### [Measurement Properties]

Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	451.0	0.0458	
2	●	277.0	0.0831	

#### [Instrument Properties]

Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

#### [Attachment Properties]

Attachment: None

#### [Operation]

Threshold: 0.0010000  
Points: 4  
InterPolate: Disabled  
Average: Disabled


#### [Sample Preparation Properties]

Weight: 0.1  
Volume: 100  
Dilution: 20 ppm  
Path Length:  
Additional Information:

# Spectrum Peak Pick Report

02-04-2019 03:41:11 PM

Data Set: BEIGE A1 B-2018-182 40PPM - RawData

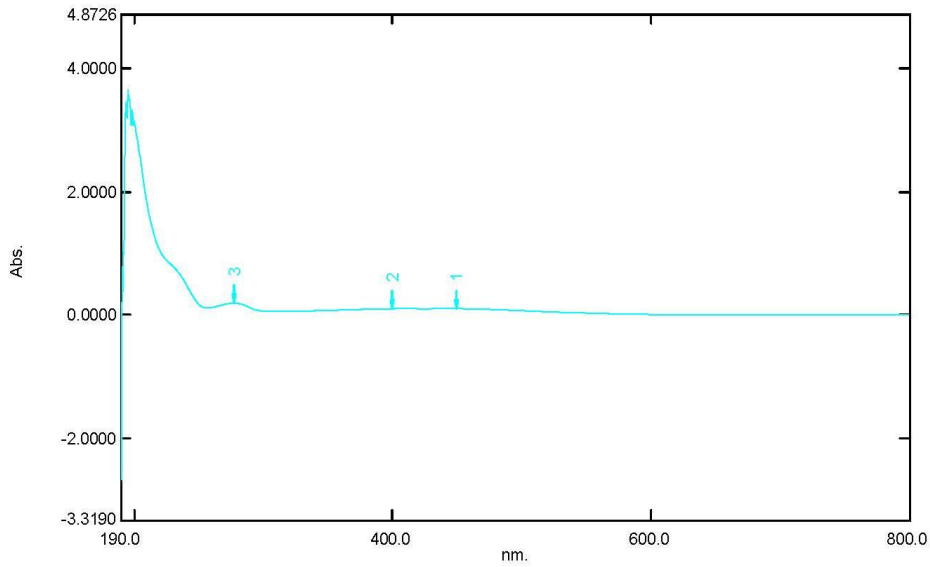

[Measurement Properties]

Wavelength Range (nm.): 190.0 to 800.0  
 Scan Speed: Fast  
 Sampling Interval: 0.5  
 Auto Sampling Interval: Enabled  
 Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	449.5	0.0983	
2	●	400.0	0.0954	
3	●	277.0	0.1867	

[Instrument Properties]

Instrument Type: UV-1900 Series  
 Measuring Mode: Absorbance  
 Slit Width: 1.0 nm  
 Light Source Change Wavelength: 340.8 nm  
 S/R Exchange: Normal

[Attachment Properties]

Attachment: None

[Operation]

Threshold: 0.0010000  
 Points: 4  
 InterPolate: Disabled  
 Average: Disabled

[Sample Preparation Properties]

Weight: 0.1  
 Volume: 100  
 Dilution: 40 ppm  
 Path Length:  
 Additional Information: