



**GREY GC**

**TOP DYEING - 3%**



**SPLIT - 3%**



**PENETRATION**



60° Solubility	Penetration	Light	<b>F A S T N E S S</b>					
			PERSPIRATION			WASHING		
			CS	SC	SW	CS	SC	SW
40	4	6	4	4	4	3	3	3

SCALE - 1 TO 5

CS - COTTON + SILK


SC - SPUN DIACETATE

SW - SPUN WOOL

# Spectrum Peak Pick Report

27-03-2019 12:25:46 PM

Data Set: GREY GC B-2018-132 10PPM - RawData

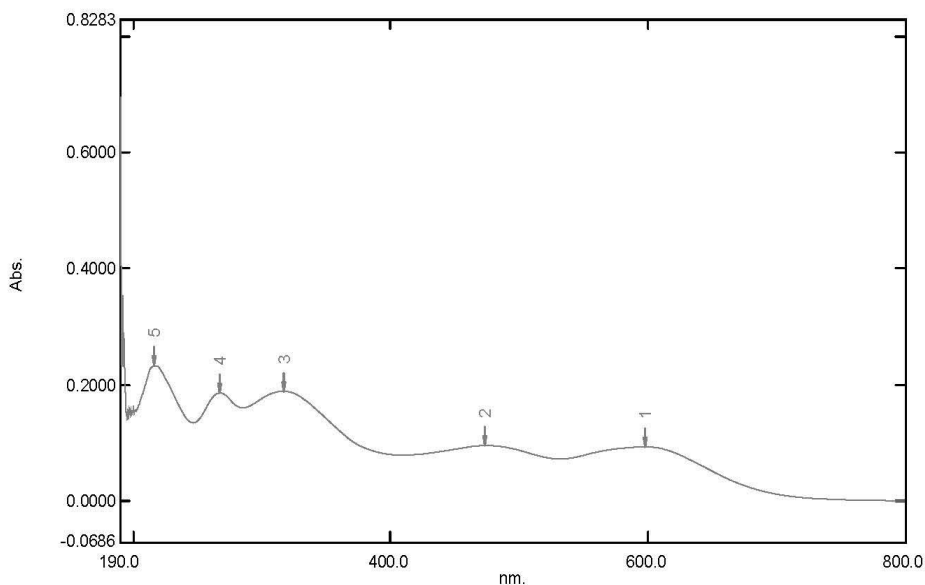

**[Measurement Properties]**

Wavelength Range (nm.): 190.0 to 800.0  
 Scan Speed: Fast  
 Sampling Interval: 0.5  
 Auto Sampling Interval: Enabled  
 Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	598.5	0.0935	
2	●	474.0	0.0957	
3	●	317.0	0.1892	
4	●	267.0	0.1864	
5	●	216.0	0.2328	

**[Instrument Properties]**

Instrument Type: UV-1900 Series  
 Measuring Mode: Absorbance  
 Slit Width: 1.0 nm  
 Light Source Change Wavelength: 340.8 nm  
 S/R Exchange: Normal

**[Attachment Properties]**

Attachment: None

**[Operation]**

Threshold: 0.0010000  
 Points: 4  
 InterPolate: Disabled  
 Average: Disabled


**[Sample Preparation Properties]**

Weight: 0.1  
 Volume: 100  
 Dilution: 10 ppm  
 Path Length:  
 Additional Information:

# Spectrum Peak Pick Report

27-03-2019 12:23:28 PM

Data Set: GREY GC B-2018-132 20PPM - RawData

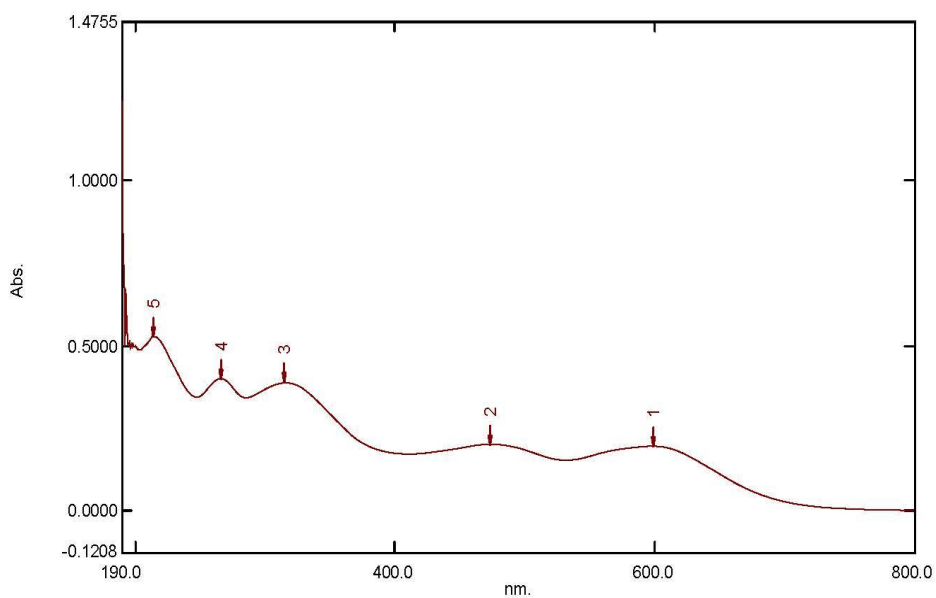

[Measurement Properties]

Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	599.5	0.1962	
2	●	474.0	0.2020	
3	●	315.0	0.3871	
4	●	265.5	0.3997	
5	●	213.5	0.5274	

[Instrument Properties]

Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

[Attachment Properties]

Attachment: None

[Operation]

Threshold: 0.0010000  
Points: 4  
InterPolate: Disabled  
Average: Disabled

[Sample Preparation Properties]

Weight: 0.1  
Volume: 100  
Dilution: 20 ppm


Path Length:

Additional Information:

# Spectrum Peak Pick Report

27-03-2019 12:14:42 PM

Data Set: GREY GC B-2018-132 40PPM - RawData

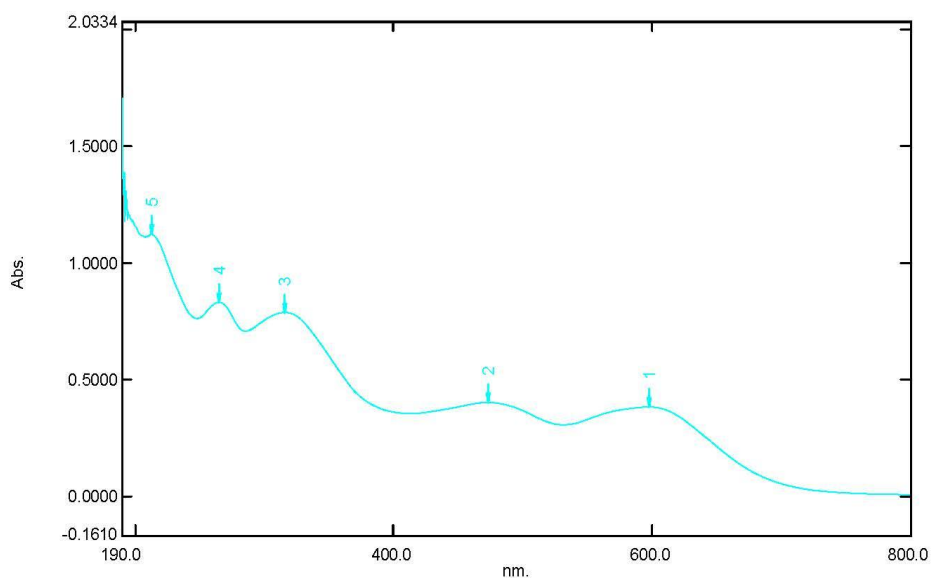

[Measurement Properties]  
Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	598.0	0.3844	
2	●	473.0	0.4036	
3	●	316.0	0.7895	
4	●	265.0	0.8325	
5	●	213.0	1.1232	

[Instrument Properties]  
Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

[Attachment Properties]  
Attachment: None

[Operation]  
Threshold: 0.0010000  
Points: 4  
InterPolate: Disabled  
Average: Disabled

[Sample Preparation Properties]  
Weight: 0.1  
Volume: 100  
Dilution: 40 ppm  
Path Length:  
Additional Information: