




## TURQ. BLUE FBL


TOP DYEING - 2%

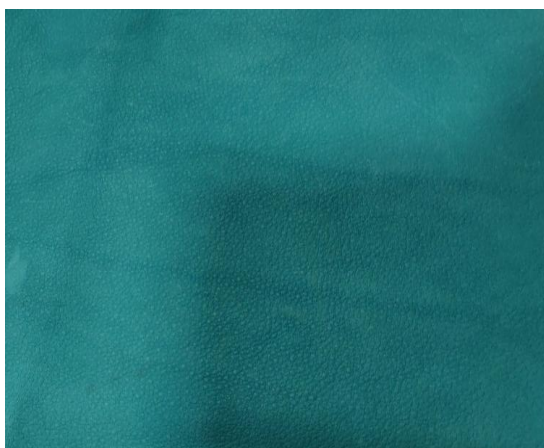

SPLIT - 3%



PENETRATION

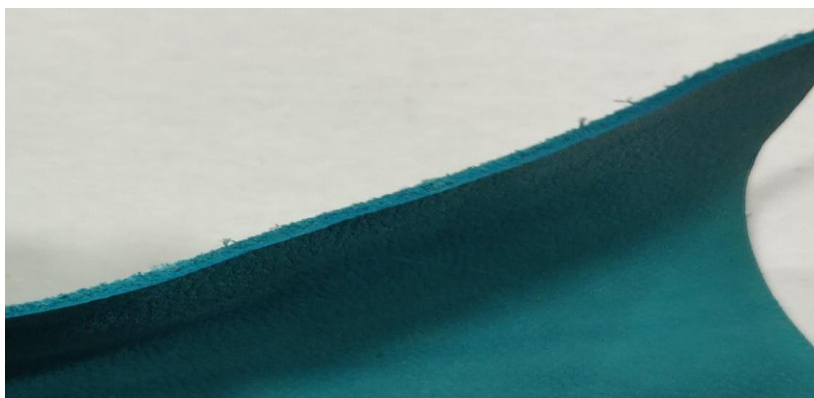

60° Solubility	Penetration	Light	F A S T N E S S					
			PERSPIRATION			WASHING		
			CS	SC	SW	CS	SC	SW
50	3	5-6	3	3	3	2	2	2

SCALE - 1 TO 5

CS - COTTON + SILK


SC - SPUN DIACETATE

SW - SPUN WOOL

# Spectrum Peak Pick Report

03-04-2019 04:22:29 PM

Data Set: TURQ BLUE FBL B-2018-188 10PPM - RawData

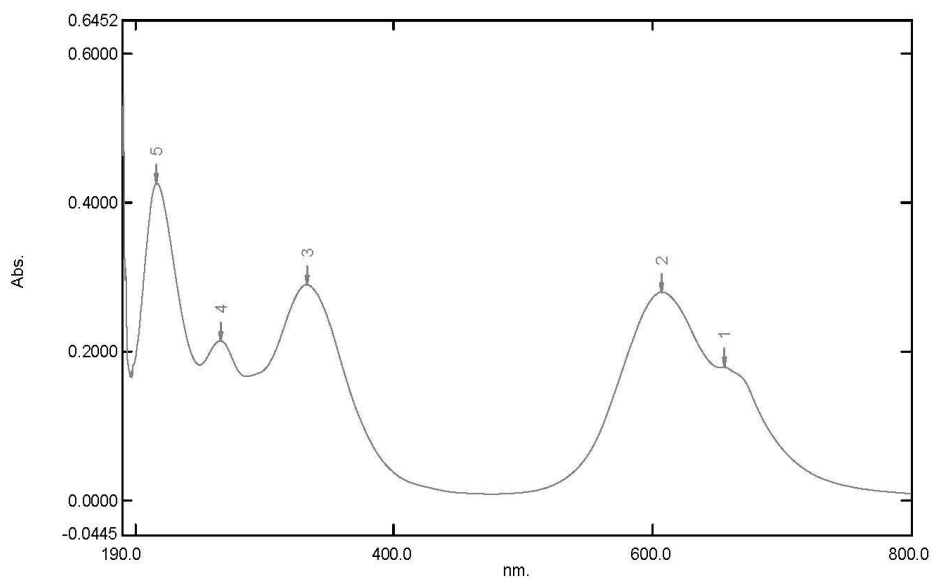

[Measurement Properties]  
Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	655.5	0.1793	
2	●	607.5	0.2800	
3	●	332.5	0.2903	
4	●	265.5	0.2145	
5	●	216.5	0.4261	

[Instrument Properties]  
Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

[Attachment Properties]  
Attachment: None


[Operation]  
Threshold: 0.0010000  
Points: 4  
InterPolate: Disabled  
Average: Disabled

[Sample Preparation Properties]  
Weight: 0.1  
Volume: 100  
Dilution: 10 ppm  
Path Length:  
Additional Information:

# Spectrum Peak Pick Report

03-04-2019 04:20:22 PM

Data Set: TURQ BLUE FBL B-2018-188 20PPM - RawData

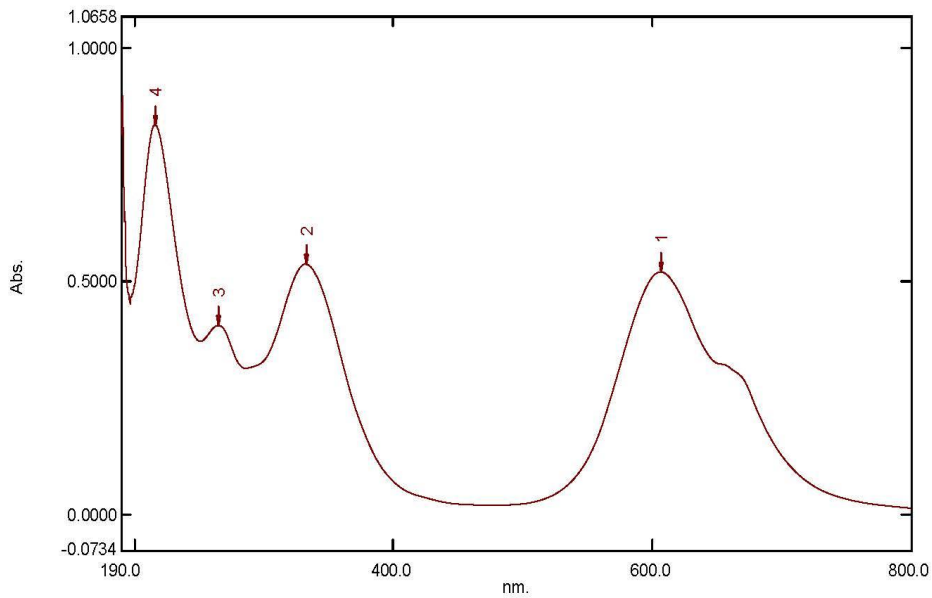

[Measurement Properties]

Wavelength Range (nm.): 190.0 to 800.0  
Scan Speed: Fast  
Sampling Interval: 0.5  
Auto Sampling Interval: Enabled  
Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	●	607.0	0.5197	
2	●	332.5	0.5367	
3	●	264.5	0.4051	
4	●	216.0	0.8349	

[Instrument Properties]

Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

[Attachment Properties]

Attachment: None

[Operation]

Threshold: 0.0010000  
Points: 4  
InterPolate: Disabled  
Average: Disabled


[Sample Preparation Properties]

Weight: 0.1  
Volume: 100  
Dilution: 20 ppm  
Path Length:  
Additional Information:

# Spectrum Peak Pick Report

03-04-2019 04:14:04 PM

Data Set: TURQ BLUE FBL B-2018-188 40PPM - RawData

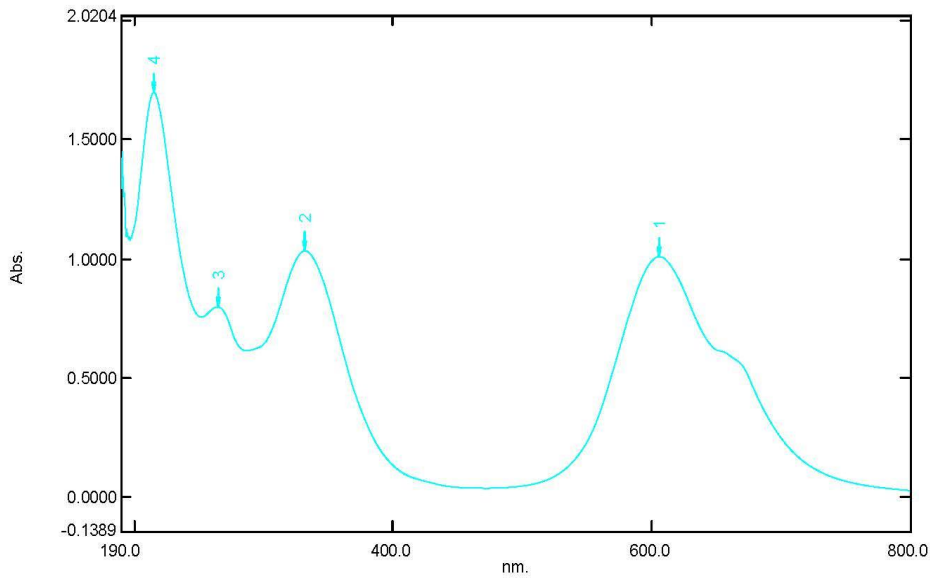

[Measurement Properties]

Wavelength Range (nm.): 190.0 to 800.0  
 Scan Speed: Fast  
 Sampling Interval: 0.5  
 Auto Sampling Interval: Enabled  
 Scan Mode: Single

No.	P/V	Wavelength	Abs.	Description
1	⊕	606.0	1.0099	
2	⊕	332.0	1.0347	
3	⊕	264.5	0.7982	
4	⊕	215.5	1.6993	

[Instrument Properties]

Instrument Type: UV-1900 Series  
 Measuring Mode: Absorbance  
 Slit Width: 1.0 nm  
 Light Source Change Wavelength: 340.8 nm  
 S/R Exchange: Normal

[Attachment Properties]

Attachment: None

[Operation]

Threshold: 0.0010000  
 Points: 4  
 InterPolate: Disabled  
 Average: Disabled

[Sample Preparation Properties]

Weight: 0.1  
 Volume: 100  
 Dilution: 40 ppm  
 Path Length:  
 Additional Information: